

**CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD**

2, Industrialna Str., Stara Zagora, 6000, Bulgaria,
Tel.: +359 42 630476; +359 42 620368; Fax: +359 42 602377;
www.ctec-sz.com e-mail: ctec@ctec-sz.com

**LABORATORY FOR TESTING OF MACHINERY, EQUIPMENT AND DEVICES**

Certificate of accreditation № 101 ЛН / 26.11.2018, valid until: 26.11.2022
Issued by EA BAS, in accordance with the requirements of BDS EN ISO/IEC 17025:2006

**TEST REPORT**

№ 2emc-19-130/30.10.2019

OBJECT TO BE TESTED: Electric and electronic equipment, appliances, devices. Luminaries.

Lighting fixture type LED Edge panel, Model: LED Edge 48W PMMA 100lm/W 6500K, ref.№ 981148100064091
(name of object to be tested, type, model, quantity, type and other)

APPLICANT FOR TEST: "Electrostart" JSCo. 3540 Varshets, 2 Republika Blvd.,

Tel.: +359 2 400 7011, fax: + 359 2 400 7012;

Application № 130/ 03.07.2019

(name of the firm – applicant, address, telephone, number and date of the test application)

METHOD OF TEST :

BDS EN 55015:2013+A1:2015 Limits and methods of measurement of radio disturbance characteristics of electrical lighting and similar equipment.

BDS EN 61000-3-2:2014 Electromagnetic compatibility (EMC).

Part 3-2: Limits – Limits for harmonic current emissions (equipment input current ≤ 16 A per phase).

BDS EN 61000-3-3:2013 Electromagnetic compatibility (EMC).

Part 3-3: Limits - Limitation of voltage changes, voltage fluctuations and flicker in public low-voltage supply systems, for equipment with rated current ≤ 16 A per phase and not subject to conditional connection.

BDS EN 61547:2010 Equipment for general lighting purposes - EMC immunity requirements

BDS EN 61000-4-2:2009 Electromagnetic compatibility (EMC).

Part 4-2: Testing and measurement techniques - Electrostatic discharge immunity test

BDS EN 61000-4-8:2010 Electromagnetic compatibility (EMC).

Part 4-8: Testing and measurement techniques - Power frequency magnetic field immunity test

BDS EN 61000-4-11:2006 Electromagnetic compatibility (EMC).

Part 4-11: Testing and measurement techniques-Voltage dips, short interruptions and voltage variations immunity tests
(number and name of the standards)

DATE OF ACCEPTANCE IN THE TEST LABORATORY: 03.07.2019

MANUFACTURER: "Electrostart" JSCo. 3540 Varshets, 2 Republika Blvd.,

Tel.: +359 2 400 7011, fax: + 359 2 400 7012;

(firm, trade mark, address)

DECLARED TECHNICAL DATA:

Rated voltage – 220-240 V AC

Rated frequency – 50-60 Hz

Rated power – 48 W

Class II

ELECTRONIC CONTROLGEAR: Electrostart 50W LED Driver 1200mA, ref.№ 170200000000034 ;

DATE OF TEST PERFORMANCE: 24.07.2019


THE HEAD OF LABORATORY:

/ T. Hristov





Copy of identification table and/or photo of tested object

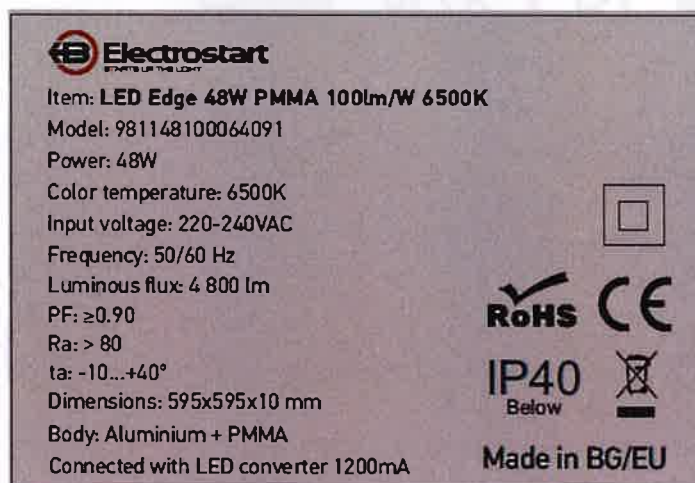

The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory





**LABORATORY FOR TESTING OF MACHINERY, EQUIPMENT AND DEVICES
CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD – Stara Zagora**

Page 3 of 14

BDS EN 55015:2013+A1:2015

Test report: № 2emc-19-130/30.10.2019

I. Emission of Radio disturbance characteristics of electrical lighting and similar equipment

1. Mains terminal disturbance voltage – 9kHz ÷ 30MHz

BDS EN 55015, cl. 4.3 – Disturbance voltage limits at mains terminals – Table 2a

BDS EN 55015, cl. 5.4 – Other luminaires

BDS EN 55015, cl. 6 – Operating conditions for lighting equipment

BDS EN 55015, cl. 6.4 – Ambient temperature: 25 °C; Relative Humidity: 42 %.

BDS EN 55015, cl.8.1 – Measuring arrangement and procedure

BDS EN 55015, cl.8.2 – Measurement of disturbance voltages, at the mains terminals of indoor and outdoor luminaires – Figure 6a.


The test is performed at supply voltage: 230 V

Measurement uncertainty: 2,75 dB(μV)

RESULTS OF MEASUREMENT :

Frequency MHz	Terminal disturbance voltages, mains line – N					
	Quasi peak - QP			Average - AV		
	Measuring dB(μV)	Margin dB(μV)	Limit dB(μV)	Measuring dB(μV)	Margin dB(μV)	Limit dB(μV)
0,052	72,34	17,23	89,57	68,10	-	-
0,155	48,90	16,83	65,73	31,16	24,57	55,73
0,220	44,16	18,66	62,82	28,08	24,74	52,82
0,355	41,67	17,17	58,84	21,95	26,89	48,84
0,360	42,62	16,11	58,73	21,83	26,90	48,73
0,495	37,17	18,91	56,08	20,74	25,34	46,08
0,505	38,96	17,04	56,00	21,47	24,53	46,00
1,000	34,21	21,79	56,00	18,71	27,29	46,00
1,890	35,39	20,61	56,00	26,27	19,73	46,00
2,155	32,37	23,63	56,00	21,02	24,98	46,00
2,915	29,83	26,17	56,00	17,16	28,84	46,00
3,120	30,34	25,66	56,00	17,46	28,54	46,00
4,915	28,25	27,75	56,00	17,61	28,39	46,00
5,355	36,17	23,83	60,00	28,49	21,51	50,00
19,560	32,91	27,09	60,00	25,95	24,05	50,00
20,125	32,48	27,52	60,00	25,32	24,68	50,00

Drawing of terminal disturbance voltages, mains line – N

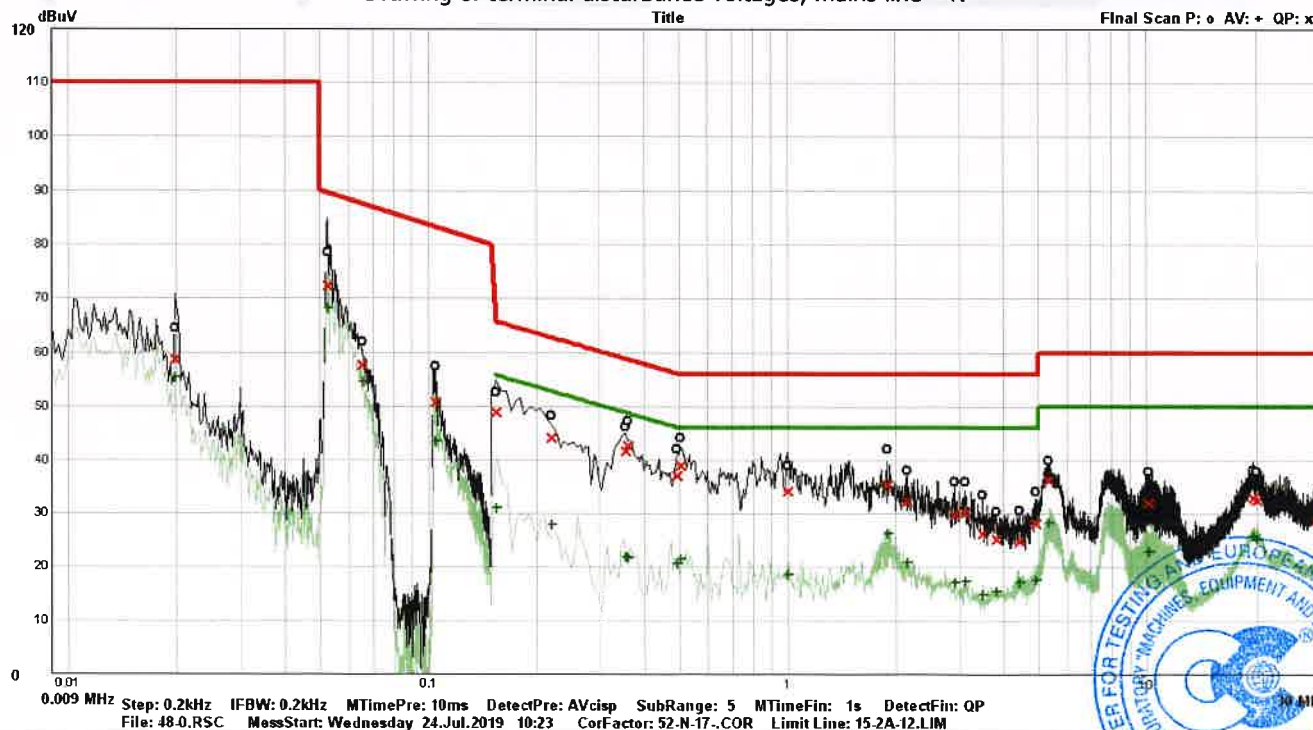

The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory





**LABORATORY FOR TESTING OF MACHINERY, EQUIPMENT AND DEVICES
CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD – Stara Zagora**


Page 4 of 14

BDS EN 55015:2013+A1:2015

Test report: № 2emc-19-130/30.10.2019

Frequency	Terminal disturbance voltages, mains line - L					
	Quasi peak - QP			Average - AV		
	Measuring	Margin	Limit	Measuring	Margin	Limit
MHz	dB(μV)	dB(μV)	dB(μV)	dB(μV)	dB(μV)	dB(μV)
0,010	76,26	33,74	110,00	73,86	-	-
0,054	76,08	13,28	89,36	69,76	-	-
0,066	56,11	31,36	87,47	53,07	-	-
0,106	51,86	31,28	83,14	47,19	-	-
0,190	51,87	12,17	64,04	35,38	18,66	54,04
0,220	45,32	17,50	62,82	29,03	23,79	52,82
0,350	41,75	17,21	58,96	25,19	23,77	48,96
0,370	41,34	17,16	58,50	26,39	22,11	48,50
0,450	38,52	18,35	56,87	17,77	29,10	46,87
0,515	40,32	15,68	56,00	20,82	25,18	46,00
1,345	39,58	16,42	56,00	23,77	22,23	46,00
1,665	36,23	19,77	56,00	22,19	23,81	46,00
2,085	35,36	20,64	56,00	24,00	22,00	46,00
2,625	30,59	25,41	56,00	18,80	27,20	46,00
3,100	29,56	26,44	56,00	17,95	28,05	46,00
3,580	26,49	29,51	56,00	16,27	29,73	46,00
3,895	27,46	28,54	56,00	17,25	28,75	46,00
4,335	25,39	30,61	56,00	16,91	29,09	46,00
4,910	28,22	27,78	56,00	19,62	26,38	46,00
5,405	36,40	23,60	60,00	28,89	21,11	50,00
10,200	34,92	25,08	60,00	25,58	24,42	50,00
29,790	26,93	33,07	60,00	19,26	30,74	50,00

Drawing of terminal disturbance voltages, mains line – L

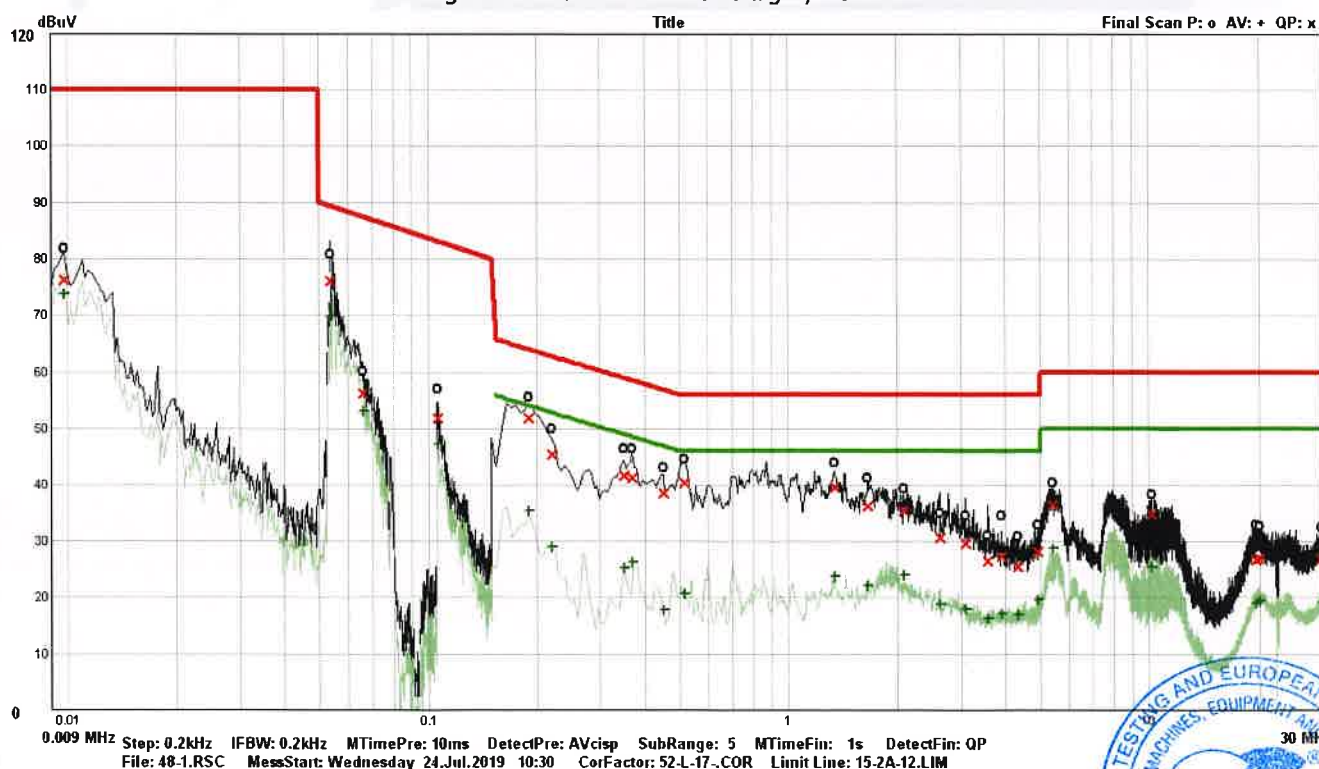

The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory





**LABORATORY FOR TESTING OF MACHINERY, EQUIPMENT AND DEVICES
CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD – STARA ZAGORA**

Page 5 of 14

BDS EN 55015:2013+A1:2015


Test report: № 2emc-19-130/30.10.2019

2. Radiated electromagnetic disturbances – 30MHz ÷ 300MHz
BDS EN 55015, cl. 4.4.2 – Frequency range 30MHz to 300MHz – Annex B. Limits - Table B.1
BDS EN 55015, cl. 5.2.4 – Other luminaires
BDS EN 55015, cl. 6 – Operating conditions for lighting equipment
BDS EN 55015, cl. 6.4 – Ambient temperature: 25 °C ; Relative Humidity: 42 %.
BDS EN 55015, cl.9.2 – Measuring arrangement and procedure related to Subclause 4.4.2
Measurement uncertainty: 3,05 dB(μV)

RESULTS OF MEASUREMENT :

Frequency	Radiated electromagnetic disturbances		
	Quasi peak - QP		
	Measuring	Margin	Measuring
MHz	dB(μV)	dB(μV)	dB(μV)
36,60	54,79	7,55	62,34
82,60	39,50	16,08	55,58
88,30	46,44	8,59	55,03
111,60	31,99	22,01	54,00
161,20	21,19	32,81	54,00
166,60	22,11	31,89	54,00
200,10	21,51	32,49	54,00
228,40	12,80	41,20	54,00
266,70	21,38	39,62	61,00
300,00	30,76	30,24	61,00

Drawing of Radiated electromagnetic disturbances

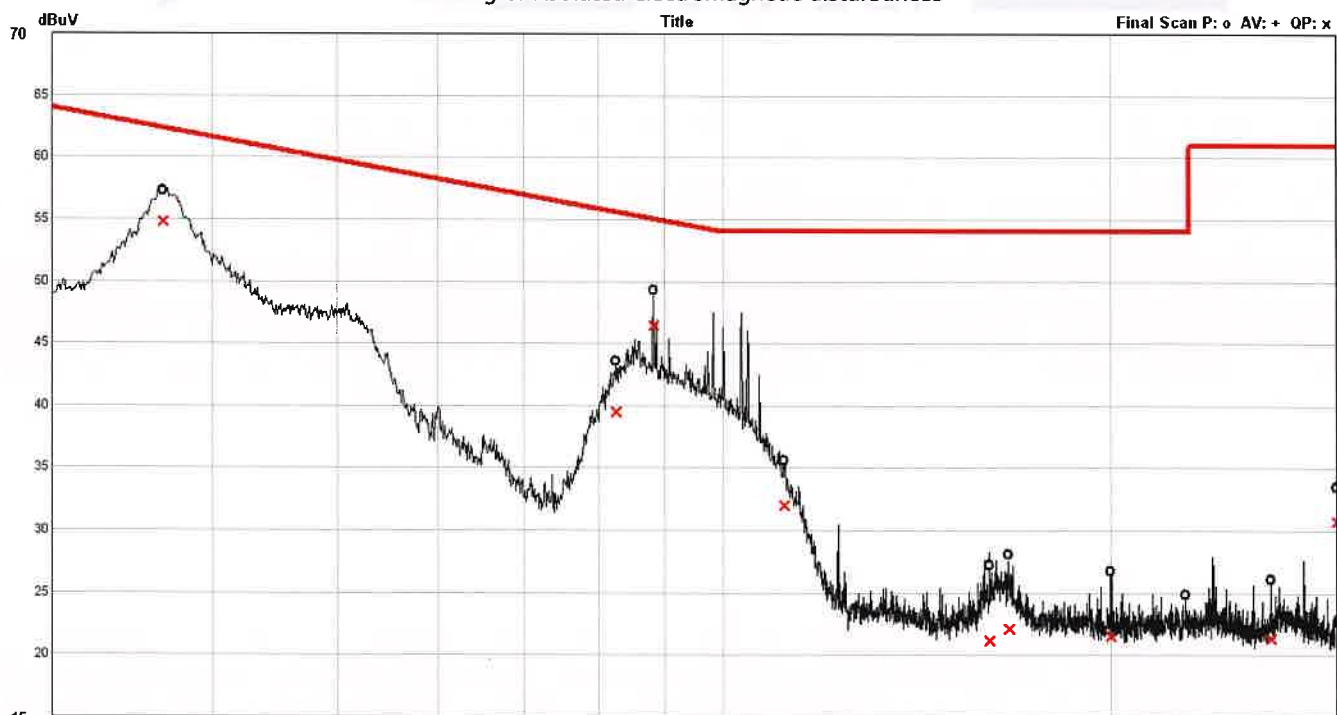

30 MHz Step: 100kHz IFBW: 120kHz MTimePre: 10ms DetectPre: Peak SubRange: 10 MTimeFin: 1s DetectFin: QP
File: 48-.RSC MessStart: Wednesday 24.Jul.2019 13:18 CorFactor: CDNM2-17.COR Limit Line: R_15_B1.LIM

300 MHz

The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory





**LABORATORY FOR TESTING OF MACHINERY, EQUIPMENT AND DEVICES
CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD – STARA ZAGORA**

Page 6 of 14

BDS EN 61000-3-2:2014

Test report: № 2emc-19-130/30.10.2019

2. HARMONIC CURRENT MEASUREMENT

Classification of equipment - C

Duration of test - 2,5 min; Measurement uncertainty: $\pm 7,1\%$

THC= 0,014692 A

I-THD= 6,973 %

POHC= 0,002288 A

POHC Limit= 0,020283 A

 $V_{RMS} = 230,0 \text{ V}$ $I_{peak} = 0,3337 \text{ A}$

Frequency = 50 Hz

 $I_{RMS} = 0,2145 \text{ A}$ $I_F = 0,2138 \text{ A}$

Power= 47,5 W

Crest Factor= 1,556

Power Factor = 0,96

K Factor= 1,288

Harmonic	AVERAGE VALUES			MAX VALUE		
	Measured	100% Limit	% of Limit	Measured	150% Limit	% of Limit
№	, A	, A	%	, A	, A	%
2	0,0013	0,0043	30	0,0013	0,0065	20
3	0,0115	0,0616	19	0,0116	0,0933	12
5	0,0059	0,0214	28	0,0060	0,0324	19
7	0,0051	0,0150	34	0,0052	0,0227	23
9	0,0018	0,0107	17	0,0019	0,0162	12
11	0,0027	0,0064	42	0,0028	0,0097	28
13	0,0016	0,0064	25	0,0016	0,0097	17
15	0,0013	0,0064	21	0,0014	0,0097	14
17	0,0007	0,0064	12	0,0008	0,0097	8
19	0,0008	0,0064	12	0,0008	0,0097	8
21	0,0008	0,0064	12	0,0008	0,0097	8
23	0,0005	0,0064	8	0,0005	0,0097	6
25	0,0008	0,0064	12	0,0008	0,0097	8
27	0,0006	0,0064	10	0,0007	0,0097	7
29	0,0005	0,0064	8	0,0005	0,0097	5
31	0,0012	0,0064	18	0,0012	0,0097	12
33	0,0004	0,0064	6	0,0004	0,0097	4
35	0,0006	0,0064	9	0,0006	0,0097	6
37	0,0006	0,0064	9	0,0006	0,0097	6
39	0,0010	0,0064	16	0,0010	0,0097	16

The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory





**LABORATORY FOR TESTING OF MACHINERY, EQUIPMENT AND DEVICES
CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD – STARA ZAGORA**

Page 7 of 14

BDS EN 61000-3-2:2014

Test report: № 2emc-19-130/30.10.2019

Harmonics of power supply source

$V_{RMS} = 230,0 \text{ V}$	$I_{peak} = 0,3337 \text{ A}$	Frequency = 50 Hz
$I_{RMS} = 0,2145 \text{ A}$	$I_F = 0,2138 \text{ A}$	Power = 47,5 W
	Power Factor = 0,96	

Harmonic	Measured	100% Limit	% of Limit
№	V	V	%
2	0,1395	0,460	30,3
3	0,2677	2,070	12,9
4	0,3044	0,460	66,2
5	0,5929	0,920	64,5
6	0,1950	0,460	42,4
7	0,0922	0,690	13,4
8	0,1610	0,460	35,0
9	0,3450	0,460	75,0
10	0,1372	0,460	29,8
11	0,1150	0,230	50,0
12	0,1150	0,230	50,0
13	0,1150	0,230	50,0
14	0,1021	0,230	44,4
15	0,0460	0,230	20,0
16	0,0920	0,230	40,0
17	0,0690	0,230	30,0
18	0,0690	0,230	30,0
19	0,0920	0,230	40,0
20	0,0692	0,230	30,1
21	0,0460	0,230	20,0
22	0,0704	0,230	30,6
23	0,1133	0,230	49,3
24	0,0690	0,230	30,0
25	0,1150	0,230	50,0
26	0,0690	0,230	30,0
27	0,0230	0,230	10,0
28	0,0690	0,230	30,0
29	0,0460	0,230	20,0
30	0,0690	0,230	30,0
31	0,1840	0,230	80,0
32	0,0690	0,230	30,0
33	0,0460	0,230	20,0
34	0,0761	0,230	33,1
35	0,0244	0,230	10,6
36	0,0690	0,230	30,0
37	0,0460	0,230	20,0
38	0,0920	0,230	40,0
39	0,1380	0,230	60,0
40	0,1150	0,230	50,0


The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory






Current and voltage waveform

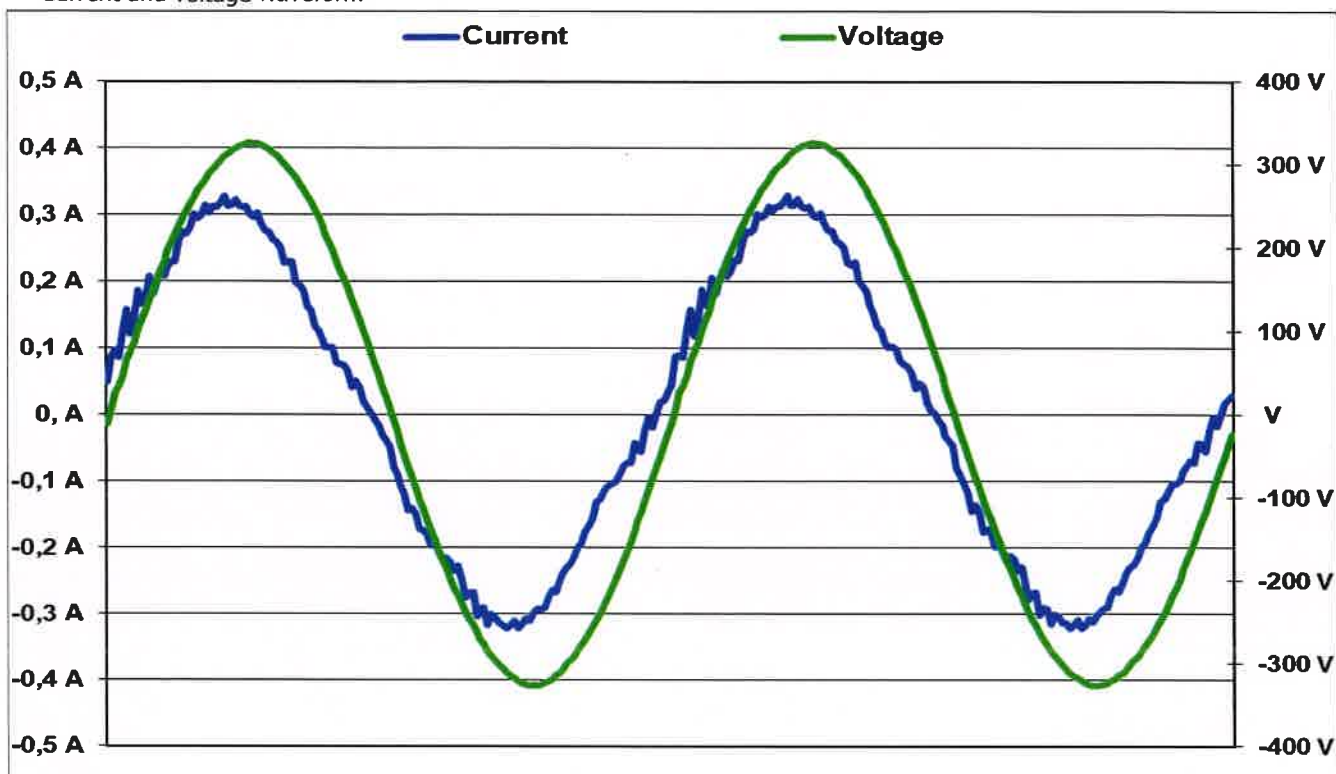

Graphics harmonics

Harmonic Currents

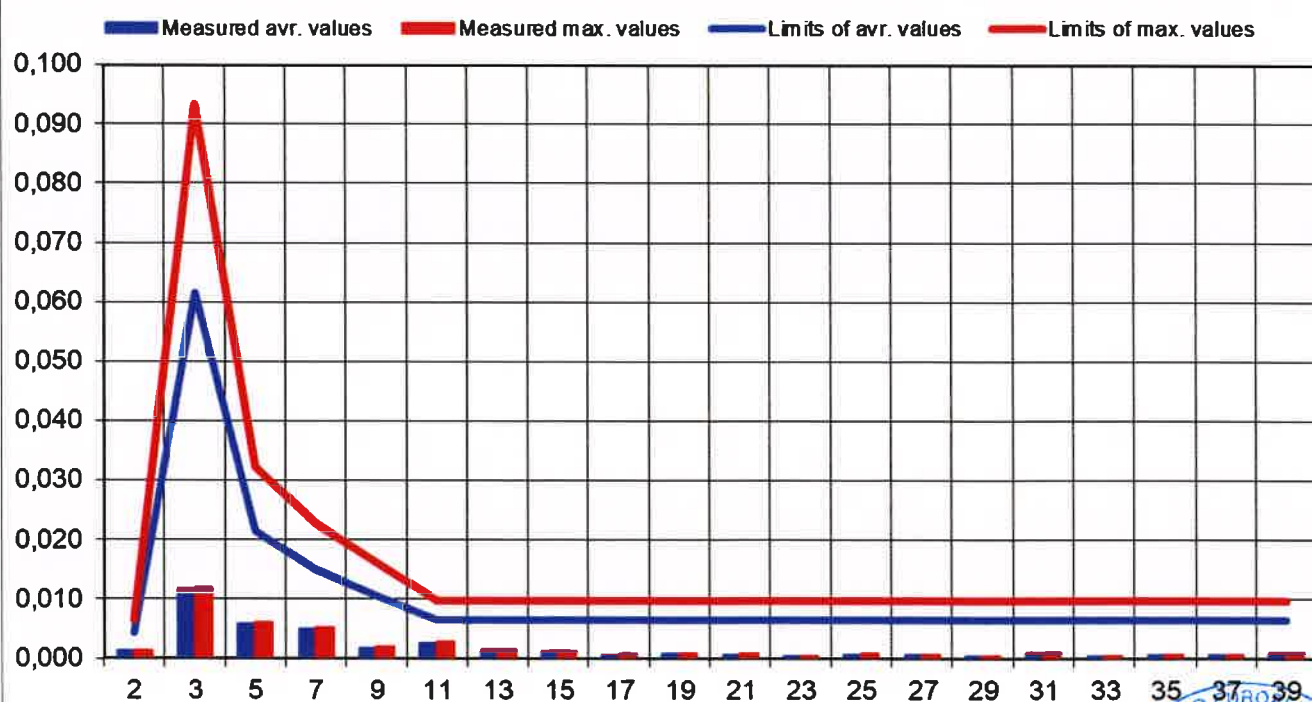

The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory





**LABORATORY FOR TESTING OF MACHINERY, EQUIPMENT AND DEVICES
CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD – STARA ZAGORA**

Page 9 of 14

BDS EN 61000-3-3:2013

Test report: № 2emc-19-130/30.10.2019

3. Voltage fluctuations and flicker measurement

EN 61000-3-3, cl. 4 – Assessment of voltage changes, voltage fluctuations and flicker

EN 61000-3-3, cl. 5 – Limits

EN 61000-3-3, cl. 6 – Test conditions

EN 61000-3-3, cl. 6.5 - Observation period

According to BDS EN 61000-3-3:2013 – Annex A, clause A.2

LED luminaires with ratings less than or equal to 200 W, are deemed to comply of limits in this standard and are not required to be tested



The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory



II. Immunity of Radio disturbance characteristics for general lighting purposes

BDS EN 61547 cl. 4.2 – Performance criteria for lighting equipment

Performance criterion A

During the test, no change of the luminous intensity shall be observed and the regulating control, if any, shall operate during the test as intended.

Performance criterion B

During the test, the luminous intensity may change to any value. After the test, the luminous intensity shall be restored to its initial value within 1 min. Regulating controls need not function during the test, but after the test, the mode of the control shall be the same as before the test provided that during the test no mode changing commands were given.

Performance criterion C

During and after the test, any change of the luminous intensity is allowed and the lamp(s) may be extinguished. After the test, within 30 min, all functions shall return to normal, if necessary by temporary interruption of the mains supply and/or operating the regulating control.

Additional requirement for lighting equipment incorporating a starting device: After the test, the lighting equipment is switched off. After half an hour, it is switched on again. The lighting equipment shall start and operate as intended.

Environment requirements during the test	Ambient temperature	15 to 35 °C
	Relative Humidity	30 to 60 %
	Air pressure	860 to 1060 mbar
Test environment	Ambient temperature	25 °C
	Relative Humidity	42 %
	Air pressure	1010 mbar




1. IMMUNITY TO ELECTROSTATIC DISCHARGE (ESD)

BDS EN 61547, cl. 5.2 – Electrostatic discharges – Table 1 - Test levels at enclosure port

BDS EN 61000-4-2, cl. 7 – Test setup

BDS EN 61000-4-2, cl. 7.2.2 – Table-top equipment , Figure 4

BDS EN 61000-4-2, cl. 8 – Test procedure

Measurement uncertainty: Tolerance of output voltage: $\pm 5\%$; Tolerance of the first peak of discharge current: $\pm 15\%$


Deviation of current rise time: $\pm 25\%$ (0,6ns – 1ns); Current deviation measured at 30ns : $\pm 30\%$

Current deviation measured at 60ns : $\pm 30\%$

Time interval between discharges	1 s
Discharge impedance	150 pF
Discharge impedance	330 Ω
Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547	Criteria B
Number of discharges	10 positive and 10 negative at the selected points

Discharge location	Type of discharge	Level	Test voltage	Polarity	Result
Body of luminaire - O	Air - Direct	1;2;3	2;4;8 kV	+	Criteria A
Body of luminaire - X	Contact - Direct	1;2	2;4 kV	+	Criteria A
Vertical coupling plane (VCP) - X	Contact - Indirect	1;2	2;4 kV	+	Criteria A
Horizontal coupling plane (HCP) - X	Contact - Indirect	1;2	2;4 kV	+	Criteria A

Picture of the object with marked points of discharge locations

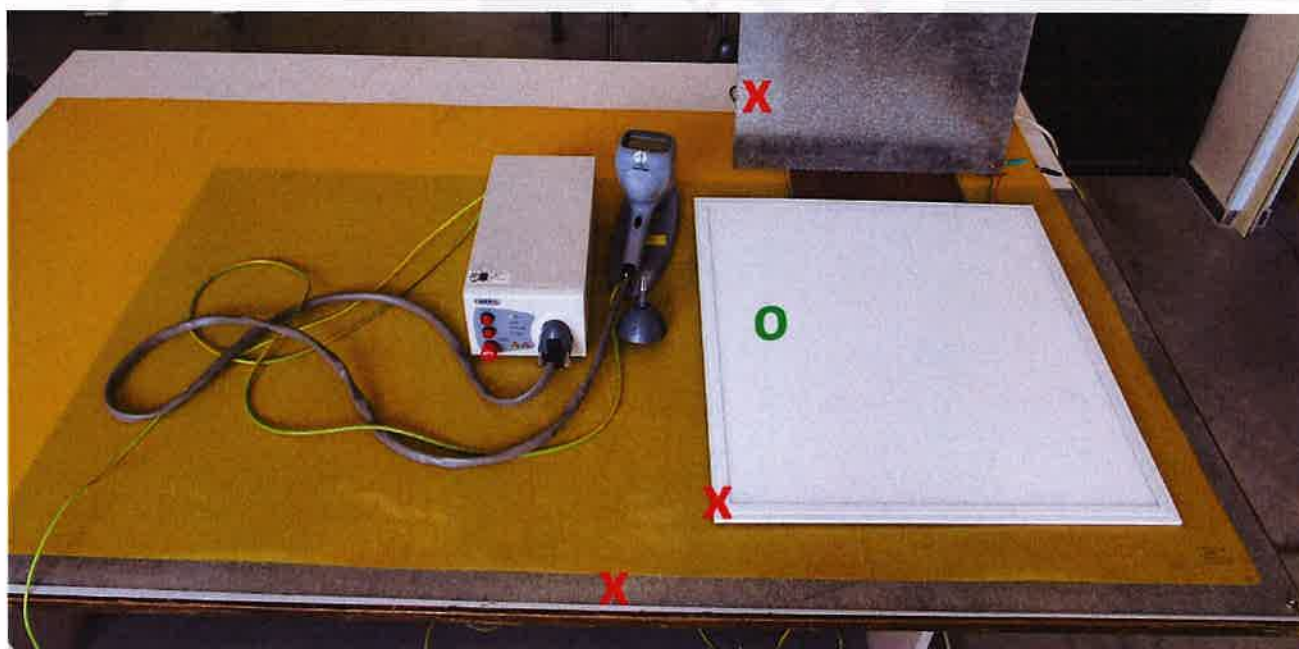

The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory




2. RATED POWER FREQUENCY MAGNETIC FIELD

BDS EN 61547, cl. 5.4 – Applicability ,Table 3

BDS EN 61000-4-8 cl. 7 – Test setup

BDS EN 61000-4-8 cl. 8 – Test procedure

Measurement uncertainty: Value of output current : $\leq 1\%$

Performance Criteria according to cl.6.3.4
and Table 15 of BDS EN 61547

Criteria A

Standard inductive coil	Orientation of standard inductive coil	Level	Field strength in the centre for all other inductive coils	Current in the coil (a coil with 10 windings)	Result
1 m x 1 m	X	2	3 A/m	3,45 A	Criteria A
1 m x 1 m	Y	2	3 A/m	3,45 A	Criteria A
1 m x 1 m	Z	2	3 A/m	3,45 A	Criteria A

The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory





3. Voltage dips, short interruptions and voltage variations immunity tests

3.1 Voltage dips immunity tests

BDS EN 61547, cl. 5.8 – Applicability ,Table 11

BDS EN 61000-4-11 cl. 7 – Test setup

BDS EN 61000-4-11 cl. 8 – Test procedure

BDS EN 61000-4-11 cl. 8.2.1 – Testing for each selected combination of test level and duration with a sequence of three dips with intervals of 10 s minimum (between each test event)

Measurement uncertainty: Deviation of output voltage : $\pm 5\%$

Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547

Criteria C

Voltage test levels (% of rated voltage)	Duration (cycles)	Phase angle synchronization	Result
70 %	10 cycles	0°	Criteria B

3.2 Short interruptions immunity tests

BDS EN 61547, cl. 5.8 – Applicability ,Table 12

BDS EN 61000-4-11 cl. 7 – Test setup

BDS EN 61000-4-11 cl. 8 – Test procedure

BDS EN 61000-4-11 cl. 8.2.1 – Testing for each selected combination of test level and duration with a sequence of three interruptions with intervals of 10 s minimum (between each test event)

Measurement uncertainty: Deviation of output voltage : $\pm 5\%$

Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547

Criteria B

Voltage test levels (% of rated voltage)	Duration (cycles)	Phase angle synchronization	Result
0 %	0,5 cycles	0°	Criteria A

The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory





**LABORATORY FOR TESTING OF MACHINERY, EQUIPMENT AND DEVICES
CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD – STARA ZAGORA**

Page 14 of 14

Test report: № 2emc-19-130/30.10.2019

USED TECHNICAL EQUIPMENTS:

	Appliance	Type	Manufacturer	Identity №	Last calibration date
1.	Digital multimeter	UNIGOR 390	LEM Austria	PI 3288	20.03.2017
2.	Voltage Generator	GL 01-16-230	Neosvet Bulgaria	0001	-
3.	Power Quality Analyzer	435	Fluke Netherlands	DM 9881064	20.10.2017
4.	Thermometer-higrometer	177-H1	TESTO Germany	01320300/902	17.04.2018
5.	EMI – receiver 9 kHz ÷ 1000 MHz	SCR 3501	Schaffner Electrotest GmbH, Germany	522	21.08.2017
6.	Line impedance stabilisation networks	NNB 52	TESEQ Switzerland	26326	15.08.2017
7.	ESD - Generator	NSG438	TESEQ Switzerland	988	12.04.2018

TEST PERFORMER: 1.

/ D. Chavalinov /



2.

/ T. Hristov /

THE HEAD OF LABORATORY :

/ T. Hristov /

The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory